

Titre: Title:	Fully automated pixel-wise myocardial blood flow quantification with first-pass perfusion CMR
Auteurs: Authors:	Li-Yueh Hsu, Matthew Jacobs, Mitchel Benovoy, Hannah Conn, & Andrew E. Arai
Date:	2016
Type:	Communication de conférence / Conference or Workshop Item
Référence: Citation:	Hsu, L.-Y., Jacobs, M., Benovoy, M., Conn, H., & Arai, A. E. (janvier 2016). Fully automated pixel-wise myocardial blood flow quantification with first-pass perfusion CMR [Présentation]. Dans 19th annual SCMR Scientific Session, Los Angeles, CA, USA (2 pages). Publié dans Journal of Cardiovascular Magnetic Resonance, 18(S1). https://doi.org/10.1186/1532-429x-18-s1-o87

 **Document en libre accès dans PolyPublie**
Open Access document in PolyPublie

URL de PolyPublie: PolyPublie URL:	https://publications.polymtl.ca/54259/
Version:	Version officielle de l'éditeur / Published version Révisé par les pairs / Refereed
Conditions d'utilisation: Terms of Use:	Creative Commons Attribution 4.0 International (CC BY)

 **Document publié chez l'éditeur officiel**
Document issued by the official publisher

Nom de la conférence: Conference Name:	19th annual SCMR Scientific Session
Date et lieu: Date and Location:	2016-01-27 - 2016-01-30, Los Angeles, CA, USA
Maison d'édition: Publisher:	BioMed Central
URL officiel: Official URL:	https://doi.org/10.1186/1532-429x-18-s1-o87
Mention légale: Legal notice:	This article is published under license to BioMed Central Ltd. This is an Open Access article distributed under the terms of the Creative Commons Attribution License (http://creativecommons.org/licenses/by/4.0), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited. The Creative Commons Public Domain Dedication waiver (http://creativecommons.org/publicdomain/zero/1.0/) applies to the data made available in this article, unless otherwise stated.

ORAL PRESENTATION

Open Access

Fully automated pixel-wise myocardial blood flow quantification with first-pass perfusion CMR

Li-Yueh Hsu^{1*}, Matthew Jacobs^{1,2}, Mitchel Benovoy^{1,3}, Hannah M Conn¹, Andrew E Arai¹

From 19th Annual SCMR Scientific Sessions
Los Angeles, CA, USA. 27-30 January 2016

Background

Fully quantitative CMR perfusion pixel maps have been validated with microsphere myocardial blood flow (MBF) measurements and shown potential clinical applications. However, the process of quantification can be time-consuming. We developed a fully automated image processing method to generate MBF pixel maps from the first-pass CMR perfusion images.


Methods

Rest and adenosine stress perfusion imaging was performed on 17 normal volunteers. A saturation recovery SSFP dual-sequence technique was used to acquire three myocardial slices and an arterial input function (AIF)

image series. A proton-density weighted image was acquired at the beginning of each series. Fully quantitative perfusion pixel maps were generated by an automated processing method, including non-rigid motion correction, surface-coil intensity correction, AIF and myocardial signal and contrast timing detection, and model constrained deconvolution. The results of the automatically generated MBF pixel maps were compared with manual quantification using an 18-segment model.

Results

MBF was compared in 612 segments from 102 perfusion image series. There was an excellent Pearson's correlation between the automated and manual perfusion pixel maps

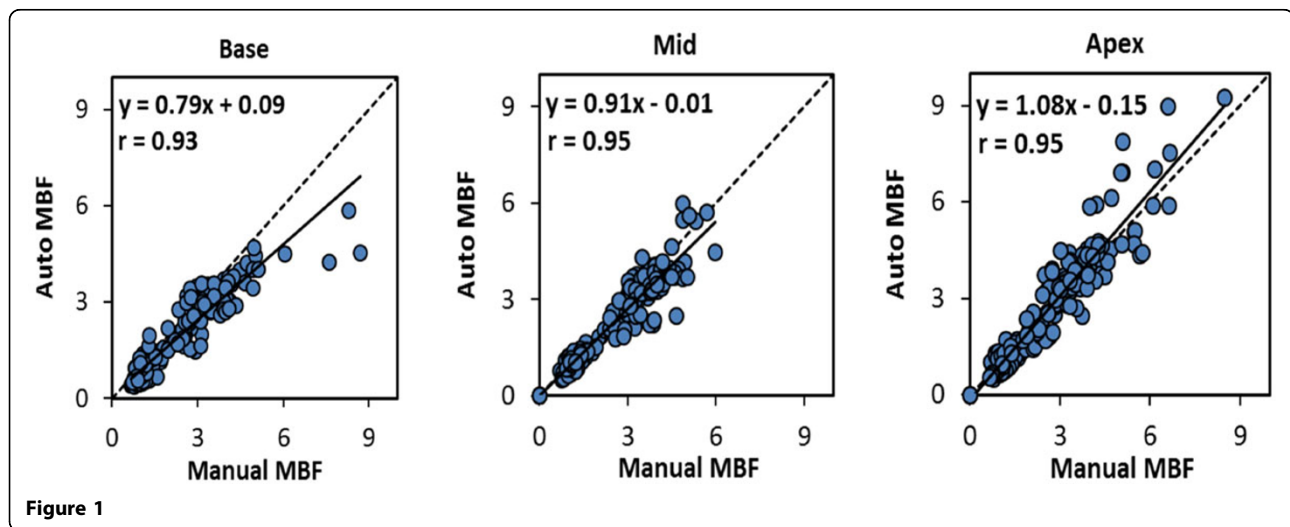

¹National Heart Lung and Blood Institute, National Institutes of Health, Bethesda, MD, USA

Full list of author information is available at the end of the article

in all slice locations ($r = 0.93, 0.95,$ and $0.95,$ figure-1). Bland-Altman analysis showed no significant bias between the two methods (bias -0.20 ml/g/min).

Conclusions

We present a fully automated pipeline for processing fully quantitative MBF maps from CMR perfusion images. Our results show the automatically generated perfusion pixel maps have a high degree of agreement compared with manual quantification.

Authors' details

¹National Heart Lung and Blood Institute, National Institutes of Health, Bethesda, MD, USA. ²Department of Electrical Engineering and Computer Science, Catholic University of America, Washington, DC, USA. ³Department of Biomedical Engineering, Polytechnique Montreal, Montreal, QC, Canada.

Published: 27 January 2016

doi:10.1186/1532-429X-18-S1-O87

Cite this article as: Hsu *et al.*: Fully automated pixel-wise myocardial blood flow quantification with first-pass perfusion CMR. *Journal of Cardiovascular Magnetic Resonance* 2016 **18**(Suppl 1):O87.

**Submit your next manuscript to BioMed Central
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

